


MAG


Quick Start Guide

MAG Front Panel

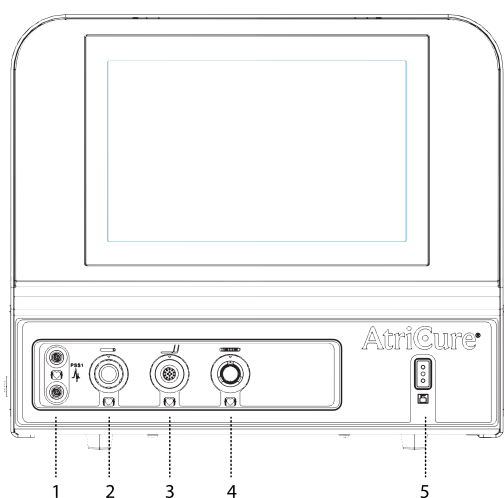


- | | |
|---------------------------|--------------------------------|
| 1. Sense-Pace Input (MLP) | 4. Epi-Sense Receptacle |
| 2. Pens Receptacle | 5. Return Electrode Receptacle |
| 3. Clamp Receptacle | |

MAG Rear Panel

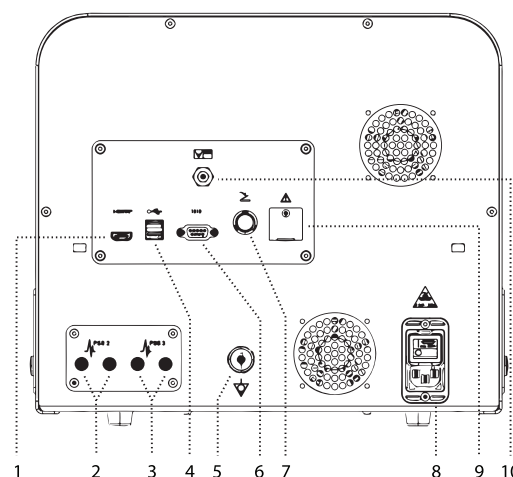

- | | |
|----------------------------|-----------------------------|
| 1. HDMI Port | 6. RS-232 Port (Future Use) |
| 2. PSS Port (EKG) | 7. Footswitch Receptacle |
| 3. PSS Port (EKG) | 8. Power Switch |
| 4. USB Port | 9. Service port (ATRC Only) |
| 5. Equipotential Connector | 10. Vacuum Port |

MAG Connections

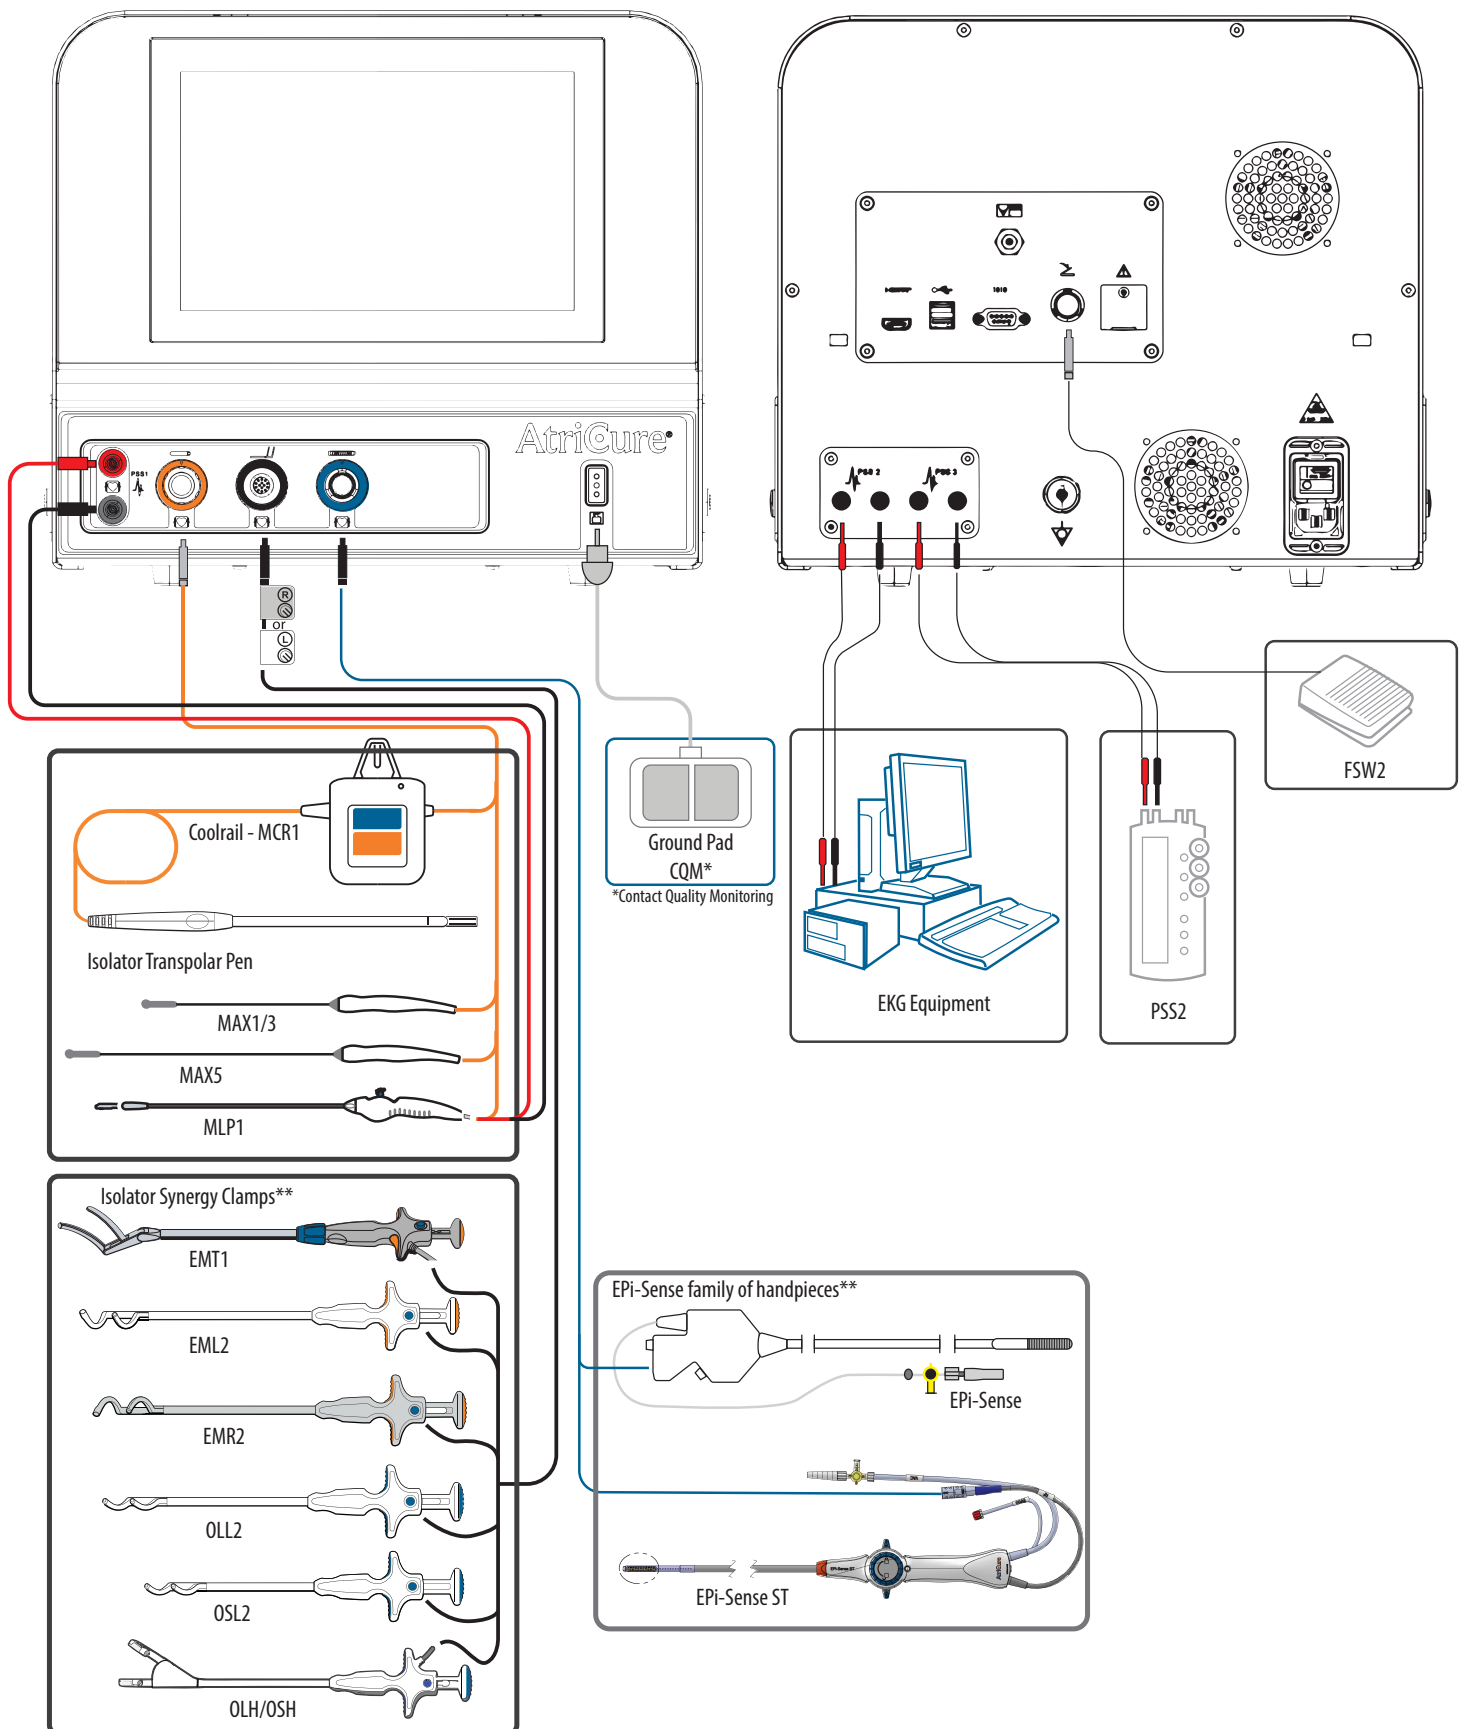

**Not all products are approved in all regions.

POWERING UP THE MAG



WARNING

CONNECT PRODUCTS TO THE MAG ONLY WHEN RF ENERGY IS OFF. FAILURE TO DO SO MAY RESULT IN AN INJURY OR ELECTRICAL SHOCK TO THE PATIENT OR OPERATING ROOM PERSONNEL.

USE GLOVES WHEN OPERATING THE MAG

1. Connect the provided power cord to the rear of the MAG.
 - Make sure that power cord is fully seated in the receptacle.
2. Plug the MAG into a grounded power outlet.
 - Do not use multiple-outlet sockets, extension cords or three-prong to two-prong adapters. Periodically check the power cord assembly for damaged insulation or connectors.
 - Ensure that access to the power cord outlet is maintained, so that the power cord can be quickly removed in the event of an emergency.
3. If using the footswitch, make sure that it is connected.
 - Pens and Clamp Handpieces: To start RF energy (to perform ablations), press and hold the footswitch. To stop RF energy, release the footswitch.
 - EPi-Sense Handpieces: To start RF energy (to perform ablations), press and release the footswitch. To stop RF energy, press and release the footswitch.
4. If using an external pacing system for emergency pacing, make sure that it is available and powered up.
5. Turn the power on using the ON/OFF switch located on the rear panel.
 - After it has been powered up, the MAG performs System Self-Tests. The Self-Tests generate two quick beeps at startup.
6. Verify that the beeps are generated.
 - If all Self-Tests pass, the MAG transitions to the STANDBY mode.
 - If any Self-Test fails, the MAG will emit a constant audible tone and will go into the FAULT mode.
7. Connect the Handpiece and any needed accessories.



Note: Touchscreen Display showing SELF-TEST

FAULT MODES

- If the MAG fails a Self-Test after it is powered up or if a non-recoverable error condition is detected at any time, the MAG enters FAULT mode. A Fault code number will be displayed on screen.
- The MAG is inoperable in the FAULT mode. RF energy is disabled during the Fault Mode.
- To clear the FAULT Mode, turn the MAG power OFF and then ON again. Cycling power will clear a fault condition and restore RF power output capability.
- Recoverable error messages will stay on the LCD display until RF energy is initiated by the footswitch, or the message is cleared from the screen. Other messages will stay on the LCD display until the error is corrected (e.g., until an expired Handpiece is removed).

TROUBLESHOOTING ERROR CODES

Recoverable Error Messages

NUMBER	CAUSE	REMEDY
1	• Power measurement problem	• Clear error and continue. • If problem persists, contact AtriCure Customer Service
5	• High impedance problem	• Check handpiece. • For EPI-Sense devices check the vacuum and Return Electrode. • If problem persists, contact AtriCure Customer Service
4	• Low impedance problem	• Check handpiece
6		• For CoolRail devices, Possible cooling problem if the LED is illuminated. • If LED is illuminated there may be a problem with the cooling system • If problem persists, contact AtriCure Customer Service
8	• Cooling fan problem	• Cycle power off and back on • If problem persists, contact AtriCure Customer Service
13	• Invalid or expired handpiece	• Reconnect or replace handpiece
14		• If problem persists, contact AtriCure Customer Service
15	• Relay problem	• Clear error and continue • If problem persists, contact AtriCure Customer Service
16	• Active device removed	• Reconnect handpiece • If problem persists, contact AtriCure Customer Service
18 & 21	• Return electrode current problem	• Check return electrode • If problem persists, contact AtriCure Customer Service
23	• Current measurement problem	• Check handpiece • For CoolRail devices, Possible cooling problem if the LED is illuminated. • If LED is illuminated there may be a problem with the cooling system • If problem persists, contact AtriCure Customer Service
24	• Return electrode contact problem	• Check return electrode • If problem persists, contact AtriCure Customer Service
25	• Power measurement problem	• Clear error and continue
26		• If problem persists, contact AtriCure Customer Service
27	• Voltage measurement problem	• Cycle power off and back on • If problem persists, contact AtriCure Customer Service
29	• Footswitch disconnected	• Reconnect or replace footswitch • If problem persists, contact AtriCure Customer Service
30	• Invalid or expired handpiece	• Reconnect or replace handpiece • If problem persists, contact AtriCure Customer Service
32	• Incorrect Return Electrode	• Replace solid return electrode with a split return electrode • If problem persists, contact AtriCure Customer Service

Warning Messages

NUMBER	CAUSE	REMEDY
1	• Handpiece close to expiration	• Less than 1 hour remaining
2	• Return electrode detaching from patient	• Re-apply or replace the return electrode
3	• Footswitch connected during an ablation	• Restart ablation
4	• Ablation attempted while in sense mode	• Switch to ablate mode before attempting an ablation

Non-Recoverable Error Messages

NUMBER	CAUSE	REMEDY
1	• Internal RF Problem	• Cycle power off and back on
2		• If problem persists, contact AtriCure Customer Service
3	• Internal temperature problem	• Cycle power off and back on
4		• If problem persists, contact AtriCure Customer Service
5	• 24V power problem	• Cycle power off and back on
		• If problem persists, contact AtriCure Customer Service
6	• Footswitch Self-Test problem	• Disconnect Footswitch, cycle power off and back on
		• If problem persists, contact AtriCure Customer Service
7	• Measurement system problem	• Cycle power off and back on
		• If problem persists, contact AtriCure Customer Service
8	• High lesion temperature detected	• Cycle power off and back on
		• If problem persists, contact AtriCure Customer Service
10-18	• Internal communication problem	• Cycle power off and back on
		• If problem persists, contact AtriCure Customer Service.
19	• Real time clock problem	• Cycle power off and back on
		• If problem persists, contact AtriCure Customer Service

For other concerns, consult the Multifunctional Ablation Generator (MAG) Instructions for Use or contact the AtriCure Customer Service Hotline at (866) 349-2342.

For detailed information, please consult the Instructions for Use.



Rx ONLY

 **Caution: Federal law (US) restricts this device to sale by or on the order of a physician.**

For other concerns, consult the Multifunctional Ablation Generator (MAG) Instructions for Use or contact the AtriCure Customer Service Hotline at (866) 349-2342.

For detailed information, please consult the Instructions for Use.



AtriCure Inc.
7555 Innovation Way
Mason, Ohio 45040 USA
+1 866 349 2342
+1 513 755 4100

Australian Sponsor Name:
AA-Med Pty. Ltd.
Address:
Suite 22.02, 101 Miller Street
North Sydney NSW 2060
Australia
Tel: 1300 887 807



European Representative:
AtriCure Europe B.V.
De entree 260
1101 EE Amsterdam
NL
+31 20 7005560
ear@atricure.com



Commercial Name: Multifunctional Ablation Generator (MAG)
Technical Name: RF Ablation Equipment
Contents:
Unit IFU(s)
01 Unit of the Multifunctional Ablation Generator
01 Unit Footswitch
01 Unit Power Cord

ANVISA Registration n°: 80117581115

Registration Holder: Emergo Brazil Import
Importação e Distribuição de Produtos
Médicos Hospitalares Ltda. Avenida Francisco
Matarazzo, 1.752, Salas 502/503, Água
Branca, São Paulo-SP, CEP – 05001-200 CNPJ:
04.967.408/0001-98

Email: brazilvigilance@ul.com