

CE
2797

AtriCure® Glidepath™ Tape Instrument Guide

Instructions for Use

(GPT000, GPT200, GPT300)

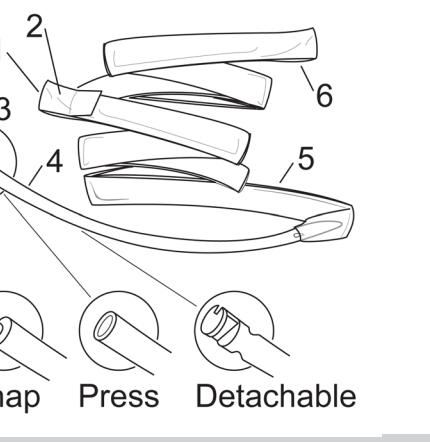


FIGURE 1



FIGURE 2

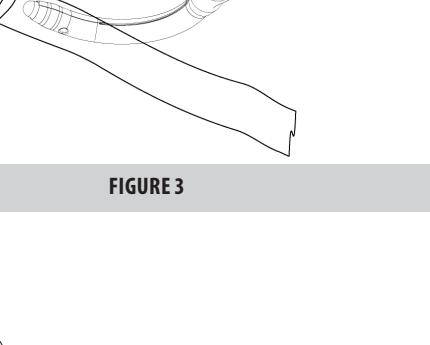


FIGURE 3

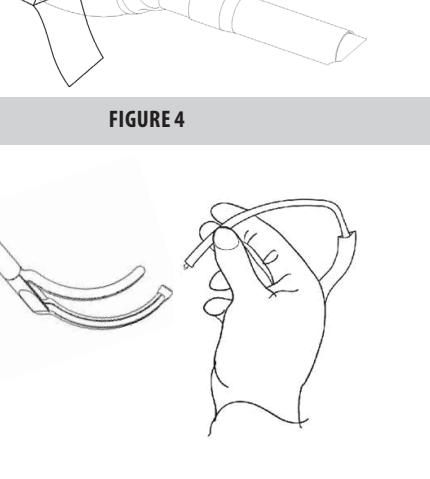


FIGURE 4

en

THIS PAGE INTENTIONALLY LEFT BLANK