

Myocardial Substrate Thickness Variability

There is great variability in substrate thickness, especially on the posterior wall.

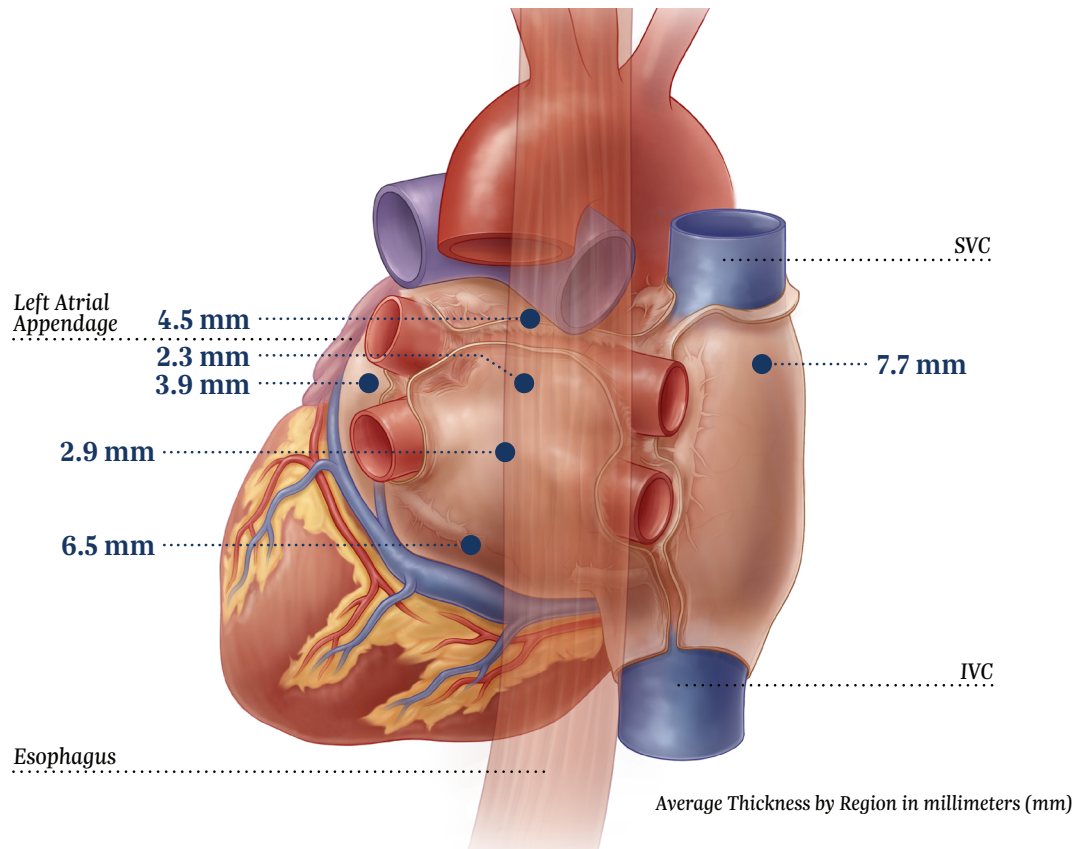


Figure 1

Melby, S.J., Schuessler, R.B., & Damiano, R.J., Jr. (2013). Ablation Technology for the Surgical Treatment of Atrial Fibrillation. *American Society for Artificial Internal Organs (ASAIO) Journal*, 59(5):461-8.

Sánchez-Quintana, D. et al. (2014). Left Atrial Anatomy Relevant to Catheter Ablation. *Cardiology Research and Practice*, DOI:10.1155/2014/289720.